





IN AN EMERGENCY, PRESS THE EMERGENCY CYCLE STOP BUTTON

ONCE THE CYCLE HAS STARTED, IT CANNOT BE INTERRUPTED

BE AWARE THAT THIS WILL CAUSE THE DEVICE TO GO TO FAULT AND A SERVICE TECHNICIAN WILL BE REQUIRED TO RESET DEVICE

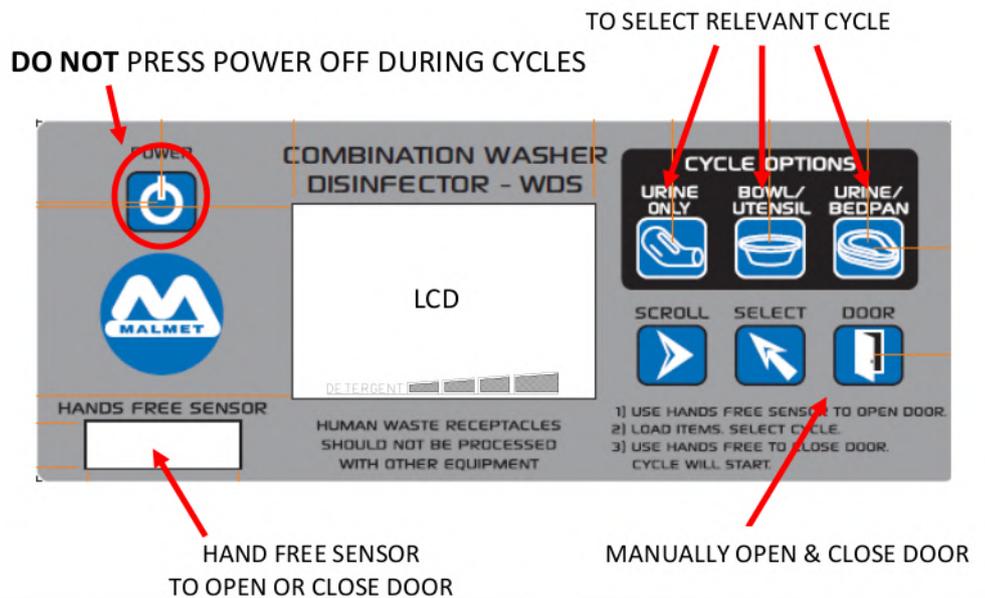

STEP 1 OPEN DOOR

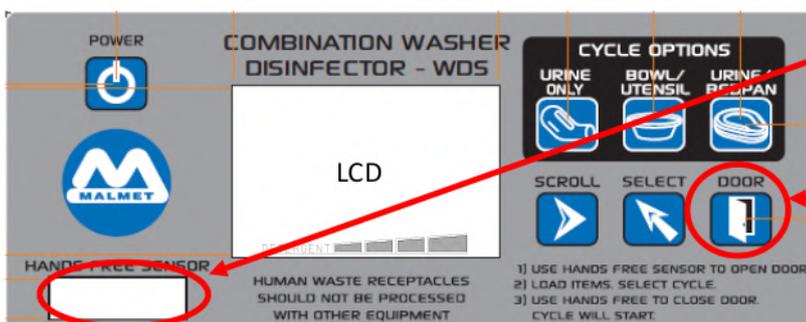



WDS INSTRUCTIONS

FOR URINAL BOTTLES ONLY



STEP 2 SET RACKS AS REQUIRED



BEDPAN RACK MUST BE IN THE DOWN POSITION



BOWL RACK MUST BE UP AGAINST BACK WALL OF CHAMBER

STEP 3 LOAD URINAL BOTTLES



STEP 4 SELECT & START CYCLE



PRESS THE RELEVANT CYCLE BUTTON TO START CYCLE.

HANDS FREE SENSOR



ACTIVATE SENSOR TO CLOSE DOOR AND AGAIN WHILST "START" IS FLASHING TO START CYCLE



WDS INSTRUCTIONS

FOR BOWLS AND/OR UTENSILS



STEP 2 SET RACKS AS REQUIRED



BEDPAN RACK MUST BE IN THE DOWN POSITION



BOWL RACK MUST BE IN DOWN POSITION

STEP 3 LOAD BOWLS AND/OR UTENSILS



KIDNEY DISHES ON KIDNEY DISH RACK



LARGE BOWLS



MEDIUM BOWLS

STEP 4 SELECT & START CYCLE



PRESS THE RELEVANT CYCLE BUTTON TO START CYCLE.

HANDS FREE SENSOR



ACTIVATE SENSOR TO CLOSE DOOR AND AGAIN WHILST "START" IS FLASHING TO START CYCLE



WDS INSTRUCTIONS

FOR URINAL BOTTLES AND/OR BEDPANS



STEP 2 SET RACKS AS REQUIRED




BEDPAN RACK UP & LOCKED IN POSITION




BOWL RACK MUST BE UP AGAINST BACK WALL OF CHAMBER

STEP 3 LOAD URINAL BOTTLES AND/OR BEDPANS

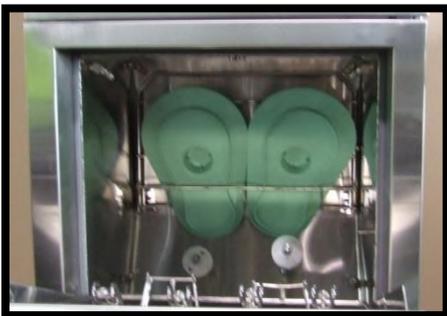

BEDPAN LIDS INTO BACK OF BOWL RACK

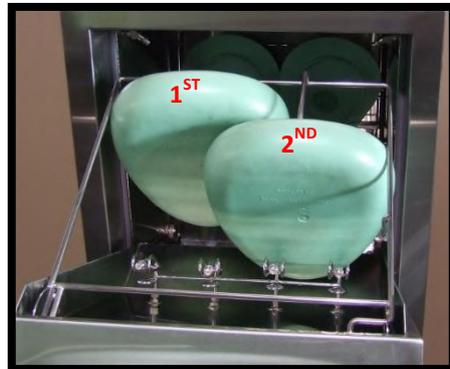

BEDPAN OR SLIPPER PANS ONTO BOTTOM HOLDER OF RACK



URINAL BOTTLES IN RACK

STEP 4 SELECT & START CYCLE



PRESS THE RELEVANT CYCLE BUTTON TO START CYCLE.

HANDS FREE SENSOR



ACTIVATE SENSOR TO CLOSE DOOR AND AGAIN WHILST "START" IS FLASHING TO START CYCLE